

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau



B2


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : <b>A61B 17/00</b>		<b>A1</b>	(11) International Publication Number: <b>WO 99/23952</b>
			(43) International Publication Date: 20 May 1999 (20.05.99)
(21) International Application Number: PCT/US98/23846		(81) Designated States: JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).	
(22) International Filing Date: 11 November 1998 (11.11.98)		<b>Published</b> <i>With international search report.</i>	
(30) Priority Data: 60/065,118 12 November 1997 (12.11.97) US			
(71)(72) Applicants and Inventors: DUBRUL, William [US/US]; P.O. Box 246, Redwood City, CA 94064 (US). FULTON, Richard, Eustis, III [US/US]; 1556 Wellington Avenue, Grand Junction, CO 81501 (US).			
(74) Agent: MCAULAY, Lloyd; McAulay Nissen Goldberg Kiel & Hand, LLP, 261 Madison Avenue, New York, NY 10016 (US).			

(54) Title: BIOLOGICAL PASSAGEWAY OCCLUSION REMOVAL

(57) Abstract

A device for the removal of a blockage in a passageway such as a dialysis graft (10) or in a body passageway includes a catheter for reception, aspiration of the blockage, and an occlusion engaging element (24) distal of the distal end of the catheter (16) which occlusion engaging element is supported on a wire (22) that extends through the catheter (16). At the distal end of the catheter (16), there is a device such as a multi-wing malecot expansion device (18) that is expanded after the catheter (16) is placed in position so as to block the occlusion from passing around the outside of the catheter (16). The support wire (22) can be a movable core guide wire (22) which has braided device (24) on its distal end.

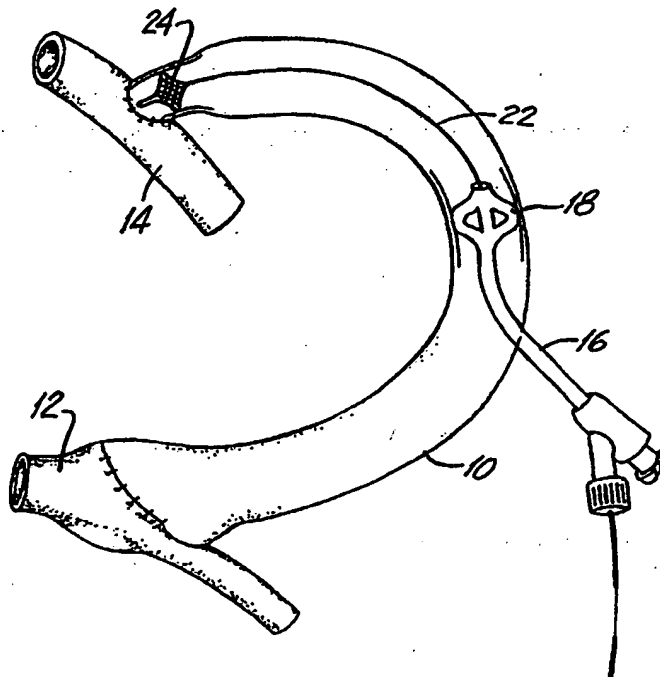

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

**BIOLOGICAL PASSAGEWAY OCCLUSION REMOVAL****Reference To Related Application**

This application claims the priority of U.S. Provisional Application, Serial No. 60/065118, filed on November 12, 1997.

5

**Background Of The Invention**

In general, this invention relates to a removal device for a biological occlusion and more particularly to a catheter and occlusion engaging element which is adapted to the removal of blockages in hemodialysis grafts.

There are many techniques and devices known in the art for removing  
10 blockages in the vascular system and other passageways of the human body.

There is a continuing need for improved devices to meet at least the following objectives.

The first objective is to reduce cost. This is particularly important in recent years where it is clear for safety and sanitary reasons that these will be single use devices. A  
15 device, even though it performs a function in some improved manner, will not be widely used if it is considerably more costly than the alternatives available.

A second objective is to provide a device that is simple to use and in a very real sense simple to understand. This will encourage its adoption and use by medical personnel. It will also tend to keep cost low.

20 The third objective is to provide a device that entails a procedure with which the medical profession is familiar so that the skills that have been learned from previous experience will continue to have applicability.

A fourth objective relates to the effectiveness and thoroughness with which the blockage is removed. It is important that a maximum amount of the blockage be  
25 removed; recognizing that no device is likely to provide one-hundred percent removal.

A fifth objective concerns safety; a matter which is often so critical as to trump the other considerations. It is important to avoid tissue trauma. In many circumstances, it is critically important to avoid breaking up a blockage in a fashion that leads to flushing elements of the blockage throughout the body involved.

30 There are trade-offs in design considerations to achieve the above five interrelated objectives. Extreme simplicity and a very simple procedure might over

compromise safety. Addressing all of these considerations calls for some trade-off between the objectives.

Accordingly, a major object of this invention is to provide an improved removal device for a body passageway blockage which achieves the objectives of reduced cost, enhanced simplicity, a standard procedure, high effectiveness and a high degree of safety. Most particularly, it is an object of this invention to achieve these objectives with an enhanced trade-off value for the combined objectives.

#### Brief Description

In brief, one embodiment of this invention is particularly adapted to the removal of blockages in hemodialysis grafts. That embodiment combines a catheter having a blocking feature that blocks the annulus between the catheter and the graft and a support wire having an occlusion engaging element.

The support wire extends through the catheter, through or around the occlusion and at its distal end has an annular braided element attached thereto. The support wire is a dual element support wire having a core and an annular shell that slides on the core. The distal end of the core is attached to the distal end of the annular braided element and the distal end of the shell is attached to the proximal end of the annular braided element. Thus movement of the core and shell relative to one another moves the braided element from a radially retracted position which is useful for insertion through the catheter to a radially expanded position which expands it to the sidewall of the graft. When the annular braided element is in its radially compressed state, it can be passed through the occlusion together with the rest of the wire to reside on the distal end of the occlusion. When the braided element is expanded and moved proximally (that is, in a retrograde fashion), it will engage the occlusion and force the occlusion into the catheter. Alternatively, no motion of the engaging element may be required if aspiration is applied. In this case, the engaging element acts as a seal to prevent the suction from aspiration to remove much material beyond its point of deployment in the channel.

The distal end of the catheter is proximal of the occlusion and contains a blocking mechanism that extends radially from the distal end of the catheter to the wall of the graft or body passageway. This catheter blocking element also has a radially retracted insertion state and a radially expanded blocking state. The blocking element is a multi-wing malecot type device which is covered by a thin elastomeric film or membrane.

This malecot type of device is bonded to the distal end of the catheter or an integral part of the catheter. The distal tip of the dilator, over which the catheter is inserted, has a slightly increased diameter. This tip is in the nature of a ferrule. When the dilator is removed, the ferrule abuts against the distal end of the multi-wing malecot pushing this blocking element from its radially compressed state into its radially expanded state. Alternatively, the tip of the dilator can be bonded to the catheter with a break-away bond so that when the dilator is removed, the blocking element is expanded in a similar fashion. In this radially expanded state, the malecot and its film cover blocks the annulus around the catheter so that the occluded blood or other obstruction which is being removed is forced into the catheter where it is aspirated or otherwise removed.

Conversely, it is understood that the blocking element could be fabricated from tubular braid and the engaging element could be formed from the malecot style configuration.

#### Brief Description Of The Figures

FIG. 1 is a mechanical schematic showing the device of this invention fully deployed in a plastic graft used in hemodialysis. The FIG. 1 drawing shows the blocking element at the distal end of the catheter in its radially expanded state and the occlusion engaging element at the distal end of the support wire in its radially expanded state. It is important to note that the blocking element may take a variety of shapes as would be required for the particular application. The preferred shape is likely to be a funnel shape where the larger diameter is distal to the lesser diameter that is proximal on the element. This funnel shape allows the obstruction to be more easily accepted into the catheter due to the pull/push of the engaging element, aspiration or both.

FIG. 2 is a longitudinal view of the distal portion of the support wire with a braided occlusion engaging element in its radially compressed state. This is the state where the support wire and engaging element can be inserted through the occlusion that is to be removed.

FIG. 3 shows the FIG. 2 braided occlusion engaging element in its radially expanded state, which is the state shown in FIG. 1.

FIG. 4 shows the multi-wing malecot type blocking element at the distal end of the catheter in its radially expanded state, which is the state shown in FIG. 1.

It should be noted that the scale of the FIG. 4 catheter is much reduced compared to the scale of the occlusion removal wire and braided element shown in FIGs. 2 and 3.

FIG. 5 is a longitudinal view, in partial cross-section, showing the catheter and dilator with a ferrule at the distal tip of the guide wire in a passageway having an occlusion that is to be removed.

FIG. 6 shows the next step in which the dilator is being removed thereby causing the malecot type blocking mechanism to become expanded by virtue of pressure against the distal end of the catheter tip of the dilator.

FIG. 7 shows the next step in which the support wire together with the braided occlusion removal element in its radially compressed state (the state shown in FIG. 2) is inserted through the catheter and through the occlusion to be removed.

FIG. 8 shows the next step in which the braided occlusion removal element has been expanded and is being pulled in a proximal direction thereby forcing the occlusion into the catheter for removal with or without aspiration.

FIG. 9 shows the multi-wing malecot type blocking element at the distal end of the catheter in its radially expanded state in accordance with another embodiment of the present invention.

FIG. 10 shows the shape of the expansion resulting from the malecot type blocking element shown in Fig. 9.

#### Description Of The Preferred Embodiments

FIG. 1 shows a typical synthetic graft 10 used in hemodialysis. The graft extends between a vein 12 and an artery 14. The graft 10 may be about thirty centimeters long with an inner diameter (I.D.) of 6 or 7 millimeters. A catheter 16 is inserted through the wall of the graft or vessel. Typically the catheter might have an outside diameter (O.D.) of 2.7 mm and an inner diameter (I.D.) of 2.3 mm. A malecot type expansion device 18 is covered with a membrane 20 (see FIG. 4). When expanded, it serves to block the annular space between the outside wall of the catheter 16 and the graft 10. A support wire 22 for a braided removal mechanism 24 will typically have an outside diameter of about one mm and has an internal actuator rod 26 (see FIG. 2) of approximately 0.5 mm. Because of the simplicity of the design, this outside diameter could be smaller than 0.5 mm. In FIG. 1, the malecot type blocking device 18 and the braided removal device 24 are both shown in their expanded state and are positioned so that retrograde or proximal movement of the support

wire 22 will pull the braided element in a proximal direction to push out whatever coagulated blood is between the braided device 18 and the distal end of the catheter into the catheter opening where it can be aspirated; thereby clearing the blockage in the graft or other vessel.

More particularly, one embodiment of this invention which has been partly  
5 tested, was designed for use in a hemodialysis graft 10 having an I.D. of approximately six to seven mm. In that case, the catheter 16 has a 8 French O.D. (2.7 mm) and a 7 French I. D. (2.3 mm). The support wire 22 is a fairly standard movable core guide wire of 35 mils (that is, 0.35 inches, which is slightly under 1 mm). The actuator rod 26 in the support wire is approximately 15 mils and thus slightly under 0.5 mm. The braided element 24 has an  
10 insertion diameter that is approximately one mm and expands to cover the seven mm diameter of the graft. In order to achieve this seven fold increase in diameter, the braided element has a length of 11 to 13 mm. Thus the catheter has an annulus of about 2.3 mm around the support wire, through which annulus the blood occlusion is aspirated.

FIGs. 2 and 3 illustrate the support wire 22 and braided element 24 which  
15 constitute the occlusion engaging element that is moved proximally to push the occlusion into the catheter for removal. A preferred occlusion engaging element 24 is a braided element. The braided material has to have a stiffness such that it will not collapse or fold under the pressure of the occlusion when this engaging element is being moved proximally. Yet the filaments that form the braid must be flexible enough to be moved between the two  
20 states as shown in FIGs. 2 and 3. Materials from polyester to stainless steel can be successfully used. A more detailed teaching of the considerations that go into the selection of the braided engaging element is set forth further on.

The distal tip of the braided element 24 is connected to the distal tip of the actuator rod 26. The proximal edge of the braided element 24 is bonded to the distal end of  
25 the support wire 22. Thus when the actuator rod 26 is pushed in a distal direction relative to the wire 22, the braided device is forced into its collapsed state shown in FIG. 2 and is available to be pushed through the catheter and through or around the occlusion which is to be removed. When this engaging element 24 has been fully inserted, the actuator rod 26 is moved in a proximal direction causing the braided element 24 to take the expanded position  
30 such as that shown in FIG. 3 so that subsequent movement of the entire support wire 22 will cause the braided element to move against the occlusion and push the occlusion into the distal end of the catheter. In some circumstances, the braided element 24 might be left as a braid with openings because the portions of the occlusion which may pass through the

- openings will be sufficiently smaller liquids so that they do not have to be removed. In other circumstances, it might be desirable to cover the braided element 24 with a membrane or film so that it becomes substantially impermeable. Further the membrane or film covering the engaging element will be helpful in preventing trauma to the inner walls of native tissue.
- 5 Even further, this membrane may be helpful in optimizing the physical characteristics of the engaging element.

With reference to FIG. 1, it might be noted that when the braided element is pushed all the way down to one end of the graft 10, as shown in FIG. 1, and then expanded it will be expanding against a portion of the wall of the graft that is smaller than the bulk of the

10 graft. However, as the support wire 22 is pulled to move the braided occlusion removal element proximally, the braided occlusion element rides on the wall of the graft and will expand as the wall of the graft expands as long as tension is maintained on the actuator rod 26.

There might be applications of the invention where the passageway involved

15 is a tissue passageway such as a blood vessel or other channel within the body, where this braided element 24 is expanded to nearly the diameter of the vessel so that when it is moved to push out an occlusion, it will avoid trauma to the wall of the vessel. Further, the membrane on the expanding element will aid in decreasing the trauma to native vessels as described above. In such a case, the engaging element (and the blocking element) may be

20 used only as a 'seal' so that the obstruction may be removed or otherwise obliterated. This seal allows the rest of the vessel to be uncontaminated and provides for a 'closed system' for irrigation and/or aspiration and subsequent obliteration or removal of the obstruction.

FIG. 4 illustrates the catheter 16 with the malecot 18 in an expanded state on the distal end of the catheter. A membrane 20 is normally used in order to provide a

25 complete blocking or sealing function. Further, the membrane 20 may aid in locking the blocking element in a particular shape. This malecot type element is created by making longitudinal slits in the sidewall of the catheter (or an attachment bonded thereto) thereby creating links or wings that will expand when the distal end of the catheter is pushed in a proximal direction. The appropriate pushing of the proximal end of the catheter is achieved,

30 as shown in FIG. 5, by a ferrule 30 which is a standard tip on a standard dilator 28. Alternatively, the dilator 28 may be a guide wire (which is usually much longer and flexible than a dilator) for remote obstruction removal. In such an application of the present invention, the guide wire would have a ferrule type mechanism that would act like the ferrule



on the dilator. In this instance, the guide wire (with ferrule) would be inserted into the vessel to the obstruction. The catheter would then be pushed along the guide wire until it reached the ferrule which would normally be located near the distal end of the guide wire. At this point the wire would be pulled back, the ferrule would butt against the catheter and force  
5 out the blocking/sealing element. The engaging element may be used with this blocking element and it could even be the ferruled wire as well.

It should be noted that the retention catheter described in United States Patent No. 3,799,172 issued on March 26, 1974 to Roman Szpur illustrates a structure that is similar to the malecot type device 18 illustrated in FIG. 4; although in that patent it is used  
10 as a retention device whereas in this invention it is used as a blocking element.

This blocking element 18 is often called a malecot in the industry. It should be understood herein that the term malecot is used to refer in general to this type of multi-wing device.

More specifically, as shown in FIG. 5, the catheter 16 together with a dilator  
15 28 having an expanded tip 30 which is a ferrule is inserted into a vessel 32 such as the graft shown in FIG. 1. The catheter 16 and dilator 28 are inserted close to the occlusion 34 and then the dilator 28 is removed. Proximal motion of the dilator 28 causes the tip 30 to contact the distal end of the catheter 16 forcing the distal end of the catheter to put pressure on the malecot wings creating the expansion shown in FIG. 6 (and also schematically shown in FIG.  
20 1). Once this expansion has occurred, the dilator with its tip can be removed from the catheter (as shown in FIG. 6).

What then occurs is shown in FIGs. 7 and 8. As shown in FIG. 7, the support wire 22 with its braided removal element 24 is inserted in the collapsed state so that it passes through or around the occlusion 34. It should be noted that the support wire 24 may be  
25 inserted prior to the blocking catheter being inserted or after the catheter is inserted (the latter of which is illustrated in the figures). Most of the occlusions to which this invention is directed such as congealed blood in a graft will permit a support wire 22 to pass through it because the consistency is that of viscous material which can be readily penetrated. Alternatively, if the occlusion is a non viscous material such as a stone, plaque, emboli,  
30 foreign body, etc. the support wire 22 is small enough to be passed around the occlusion. Once the braided element 24 is on the distal side of the occlusion 34, the actuator rod 26 is pulled creating the expanded state for the braided device. Accordingly, distal movement of the entire support wire will cause the expanded braided device to move against the occlusion

and force it into the catheter for removal with or without aspiration. When removal of obstructions that are located some distance away from the point of access into the body such as the carotid artery via a groin access the wire 22 would likely be inserted first. In this case the support wire 22 with its expanding element 24 may be used as a guide wire to guide the catheter to the preferred location. Of further import is that the blocking element and the engaging element may be used without any relative motion once deployed. Such is the case when irrigation and/or aspiration is used for the obstruction removal. In this case the two elements can be used as seals against the tubular inner walls on both sides of the obstruction whereby the obstruction is removed from that 'sealed' space with the use of aspiration, irrigation, or both. Further other means of obliterating the obstruction within this 'sealed' space may be employed. Some of those means are, but are not limited to the addition of dissolving agents, delivery of energy such as ultrasound, laser or light energy, hydraulic energy and the like.

#### The Tubular Braid Engaging Element

The engaging apparatus includes an elongate tube; an elongate mandril inside the tube and an expandable tubular braid. The elongate mandril extends from the proximal end of the device to the distal end. The elongate tube extends from close to the proximal end of the device to close to the distal end. The distal end of the tubular braid is bonded to the distal end of the inner elongate mandril. The mandril may extend beyond the tubular braid. The proximal end of the tubular braid is bonded to the distal end of the elongate tube.

The braid may be open, but may be laminated or covered with a coating of elastic, generally inelastic, plastic or plastically deformable material, such as silicone rubber, latex, polyethylene, thermoplastic elastomers (such as C-Flex, commercially available from Consolidated Polymer Technology), polyurethane and the like. The assembly of tube, mandril and braid is introduced percutaneously in its radially compressed state. In this state, the outside diameter of the braid is close to the outside diameter of the elongate tube. This diameter is in the range of 10 to 50 mils, and usually 25 to 40 mils (i.e. thousandth of an inch). After insertion, the tubular braid is expanded by moving the mandril proximally with respect to the tube.

The tubular braid is preferably formed as a mesh of individual non-elastic filaments (called "yarns" in the braiding industry). But it can have some elastic filaments interwoven to create certain characteristics. The non-elastic yarns can be materials such as polyester, PET, polypropylene, polyamide fiber (Kevlar, DuPont), composite filament wound

polymer, extruded polymer tubing (such as Nylon II or Ultem, commercially available from General Electric), stainless steel, Nickel Titanium (Nitinol), or the like so that axial shortening causes radial expansion of the braid. These materials have sufficient strength so that the engaging element will retain its expanded condition in the lumen of the body while removing the obstruction therefrom.

The braid may be of conventional construction, comprising round filaments, flat or ribbon filaments, square filaments, or the like. Non-round filaments may be advantageous to decrease the axial force required for expansion to create a preferred surface area configuration or to decrease the wall thickness of the tubular braid. The filament width or diameter will typically be from about 0.5 to 25 mils, usually being from about 5 to 10 mils. Suitable braids are commercially available from a variety of commercial suppliers.

The tubular braids are typically formed by a "Maypole" dance of yarn carriers. The braid consists of two systems of yarns alternately passing over and under each other causing a zigzag pattern on the surface. One system of yarns moves helically clockwise with respect to the fabric axis while the other moves helically counter-clockwise. The resulting fabric is a tubular braid. Common applications of tubular braids are lacings, electrical cable covers (i.e. insulation and shielding), "Chinese hand-cuffs" and reinforcements for composites. To form a balanced, torque-free fabric (tubular braid), the structure must contain the same number of yarns in each helical direction. The tubular braid may also be pressed flat so as to form a double thickness fabric strip. The braid weave used in the tubular braid of the present invention will preferably be of the construction known as "two dimensional, tubular, diamond braid" that has a 1/1 intersection pattern of the yarns which is referred to as the "intersection repeat". Alternatively, a Regular braid with a 2/2 intersection repeat and a Hercules braid with an intersection repeat of 3/3 may be used. In all instances, the helix angle (that being the angle between the axis of the tubular braid and the yarn) will increase as the braid is expanded. Even further, Longitudinal Lay-Ins can be added within the braid yarns and parallel to the axis to aid with stability, improve tensile and compressive properties and modulus of the fabric. When these longitudinal "Lay-In" yarns are elastic in nature, the tubular braid is known as an elastic braid. When the longitudinal yarns are stiff, the fabric is called a rigid braid. Biaxially braided fabrics such as those of the present invention are not dimensionally stable. This is why the braid can be placed into an expanded state from a relaxed state (in the case of putting it into the compressive mode). Alternatively this could be a decreased/reduced (braid diameter decreases) state when put into tension

from the relaxed state. When put into tension (or compression for that matter) the braid eventually reaches a state wherein the diameter will decrease no more. This is called the "Jammed State". On a stress strain curve, this corresponds to increase modulus. Much of the engineering analysis concerning braids are calculated using the "Jammed state" of the structure/braid. These calculations help one skilled in the art to design a braid with particular desired characteristics. Further, material characteristics are tensile strength, stiffness and Young's modulus. In most instances, varying the material characteristics will vary the force with which the expanded condition of the tubular can exert radially. Even further, the friction between the individual yarns has an effect on the force required to compress and un-compress the tubular braid. For the present invention, friction should be relatively low for a chosen yarn so that the user will have little trouble deploying the engaging element. This is particularly important when the engaging element is located a significant distance from the user. Such is the case when the percutaneous entry is the groin (Femoral Artery for vascular interventions) and the point of engaging the engaging element is some distance away (i.e. the Carotid Artery in the neck). Similarly, this is true for long distances that are not vascular or percutaneous applications.

#### Other Comments

An important consideration of the invention described herein is that the support wire with its expanding element can be fabricated with a very small diameter. This is important because it allows an optimally large annular space between the wire and the inside of the catheter for maximum obstruction removal. Previous engaging elements have been used that use a balloon for the engaging element. This balloon design requires a larger shaft diameter than that of the present invention. Hence in these previous devices the annular space is not maximized as in the present invention. The term wire is used to refer to the support portion of the removal device. The material of the wire need not necessarily be metal. Further, it may be desirable to use a 'double' engaging element (i.e. two braided or malecot expanding elements separated a distance appropriate to entrap the occlusion) in the case for example where the occlusion is desired to be trapped in the vessel. The term wire is used herein to refer to a dual element device having a shell component and a core or mandril component which are longitudinally moveable relative to one another so as to be able to place the braided occlusion engaging element into its small diameter insertion state and its large diameter occlusion removal state.

Although the blocking element is described as a multi-malecot type of device, it should be understood that the blocking element may be designed in various fashions which are known in the art. See, for example, Figs. 9 and 10. As another example, an appropriately designed braid arrangement could be used as the blocking element. In that case, the catheter may have to be a dual wall catheter in which the inner and outer annular walls are able to move relative to one another in a longitudinal direction so as to place the braid used as a blocking element in its small diameter insertion state and its large diameter blocking state. Alternatively, it may be a single wall similar in design to the malecot style blocking element described previously.

10           The particular embodiment disclosed was designed for an application to remove congealed blood in a dialysis graft. For some applications, like removing clots from remote vascular areas, the blocking mechanism and engaging elements may be used only as distal and proximal seals around the device to be removed so that the clot or other obstruction can be removed with aspiration or can be obliterated with some therapy such as a chemical dissolving agent or acoustical energy or lithotripsy and the like. The residual obstruction in that case would be aspirated from the tubular catheter.

          It should be further understood that there might be a situation in which the blocking element or even the occlusion engaging element would be provided to the physician in a normal expanded state so that when the device is deployed, it would, through plastic memory or elastic memory, automatically snap into its expanded state.

What Is Claimed Is:

1. A removal device for an occlusion, comprising:  
a catheter for insertion into a body passageway, said catheter having a distal  
end,  
5 a support wire insertable through said catheter, said wire having a distal end,  
a blocking mechanism on the distal end of said catheter, said blocking  
mechanism having a radially compressed state for insertion into the body passageway and a  
radially expanded state extending near to the wall of said passageway to block passage of  
material around the outside of the distal end of said catheter,  
10 an occlusion engaging element supported on said distal end of said wire, said  
engaging element having a radially compressed state for insertion of said wire through said  
catheter and through or around whatever occlusion is to be engaged and a radially expanded  
state to engage the occlusion,  
expansion of said engaging element when positioned distally of an occlusion  
15 and subsequent proximal movement of said engaging element forcing the occlusion into said  
catheter.
2. The removal device of claim 1, wherein:  
said blocking mechanism is a multi-wing malecot style mechanism, and  
said engaging element is an annular braided segment.
- 20 3. The removal device of claim 1, wherein:  
said blocking mechanism and said engaging element are both annular braided  
segments, and  
said engaging element is one of the group of annular braided segment,  
malecot and inflatable annular balloon.
- 25 4. The removal device of claim 1, wherein said engaging element in said  
expanded state contacts the wall of the passageway in which it is inserted.
5. The removal device of claim 2, wherein said engaging element in said  
expanded state contacts the wall of the passageway in which it is inserted.

6. The removal device of claim 1, wherein said occlusion engaging element is a braided element having individual yarns sufficiently flexible to be moved between said states and sufficiently stiff to substantially hold said expanded state when removing the targeted occlusion.

5 7. The removal device of claim 6, wherein said blocking mechanism is a multi-wing malecot having an annular elastomeric film around said wings.

8. The removal device of claim 1, wherein said blocking mechanism is a multi-wing malecot having an annular elastomeric film around said wings.

10 9. The removal device of claim 1, wherein said blocking mechanism is a multi-wing malecot adapted to have a funnel shape.

10. A removal device for an occlusion, comprising  
a support wire having a distal end,  
an engaging element having a retracted insertion state and an expanded  
15 occlusion removal state, said support wire including user operable means for moving said  
removal element from said retracted state to said expanded state,  
expansion of said engaging element when positioned distally of an occlusion.

11. The removal device of claim 10, wherein said engaging element is a  
braided engaging element having individual yarns sufficiently flexible to be moved between  
20 said states and sufficiently stiff to substantially hold said expanded state when removing the  
targeted occlusion.

12. The removal device of claim 10, wherein said engaging element is a multi-wing malecot style engaging element.

13. The removal device of claim 10, wherein said engaging element, after  
25 expansion, is adapted to force the occlusion to move in a proximal direction when said  
engaging element is proximally moved.

14. A catheter for use in receiving an occlusion from a body passageway into which the catheter is placed, the improvement comprising:  
a blocking mechanism on the distal end of said catheter,  
said blocking mechanism having a radially retracted insertion state and a  
5 radially expanded blocking state,  
an actuator associated with said catheter to move said blocking mechanism from said retracted state to said expanded blocking state,  
expansion of said blocking mechanism when said catheter is inserted into a body passageway assuring that material being removed in a proximal direction from a  
10 position in said passageway that is distal of said catheter will enter the lumen of said catheter and will be blocked from the body passageway external of said catheter or to act as a seal for aspiration.

15. The catheter of claim 14, wherein said blocking mechanism is a multi-wing malecot style blocking mechanism including an annular elastomeric film around  
15 said wings.

16. The catheter of claim 14, wherein said blocking mechanism has a braided configuration.

17. A method of removing an occlusion, comprising the steps of:  
inserting a catheter into a body passageway,  
20 inserting a support wire through said catheter, said wire having a distal end and having an occlusion engaging element supported on said distal end of said wire, said engaging element having a radially compressed state for insertion of said wire through said catheter,  
inserting said engaging element in the radially compressed state through or  
25 around whatever occlusion is to be engaged, and  
radially expanding said engaging elements to a radially expanded state when said engaging element is positioned distally of said occlusion.

18. The method of claim 17, further comprising the step of proximally moving said engaging element to force the occlusion into said catheter.



19. The method of claim 17, wherein said engaging element is a braided element having individual yarns sufficiently flexible to be moved between said states and sufficiently stiff to substantially hold said expanded state when removing the targeted occlusion.

5 20. The method of claim 17, wherein said engaging element is a multi-wing malecot style mechanism.

21. The method of claim 17, wherein a blocking mechanism is coupled to a distal end of said catheter, said method further comprising the steps of providing said blocking mechanism in a radially compressed state during insertion of said catheter into the  
10 passageway, and providing said blocking mechanism in a radially expanded state extending near to the wall of said passageway after insertion of said catheter into the passageway to block passage of material around the outside of the distal end of said catheter.

22. A method of removing an occlusion, comprising the steps of:  
inserting a catheter into a body passageway, said catheter having at a distal  
15 end a blocking mechanism,  
providing said blocking mechanism in a radially compressed state during insertion of said catheter into the passageway, and  
radially expanding said blocking mechanism to a radially expanded state  
extending near to the wall of said passageway after insertion of said catheter into the  
20 passageway to block passage of material around the outside of the distal end of said catheter.

23. The method of claim 22, wherein said blocking mechanism is a multi-wing malecot style mechanism.

24. The method of claim 22, wherein the step of radially expanding said blocking mechanism is carried out by expanding said blocking mechanism into a funnel  
25 shaped mechanism.

- 25 A method of removing an occlusion, comprising the steps of:  
inserting a support wire into a body passageway, said wire having at a distal  
end a blocking mechanism,  
providing said blocking mechanism in a radially compressed state during  
5 insertion of said wire into the passageway, and  
radially expanding said blocking mechanism to a radially expanded state  
extending near to the wall of said passageway after insertion of said catheter into the  
passageway to block passage of material around the outside of the distal end of said wire.

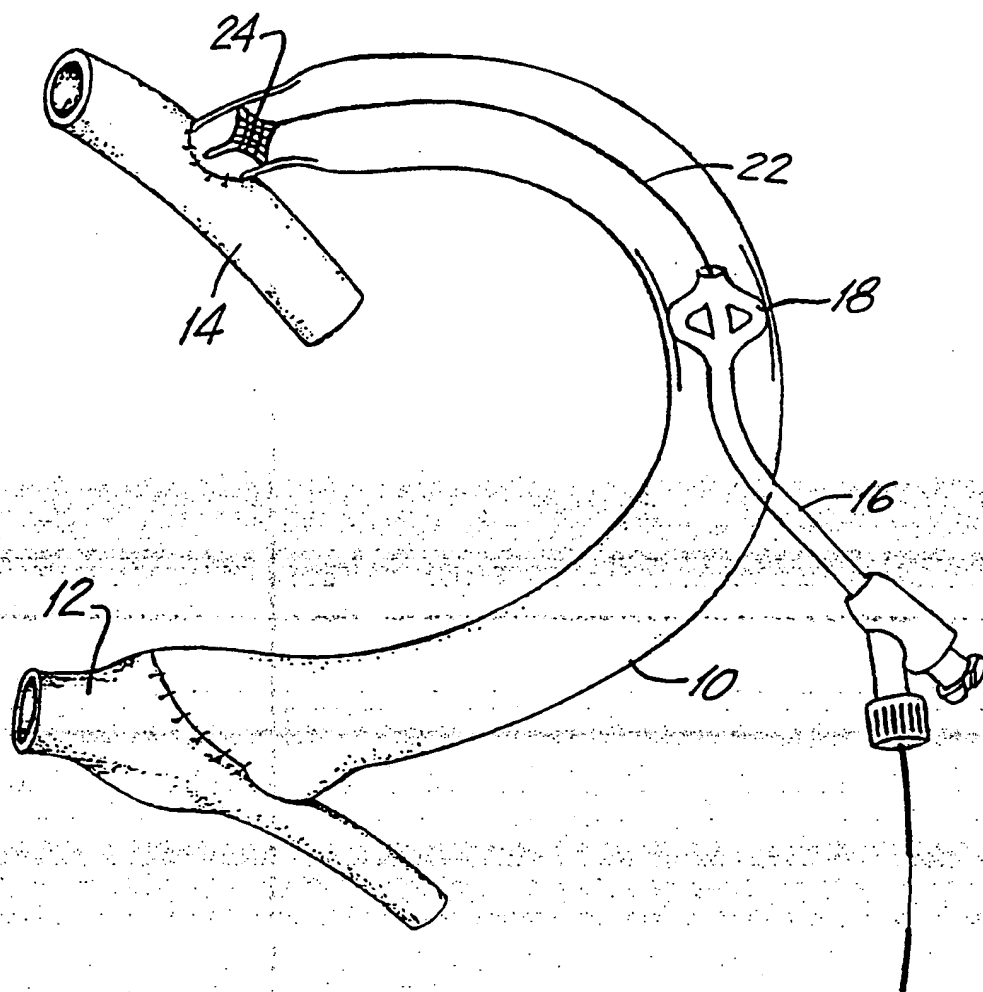


FIG. 1

2/4



FIG. 2

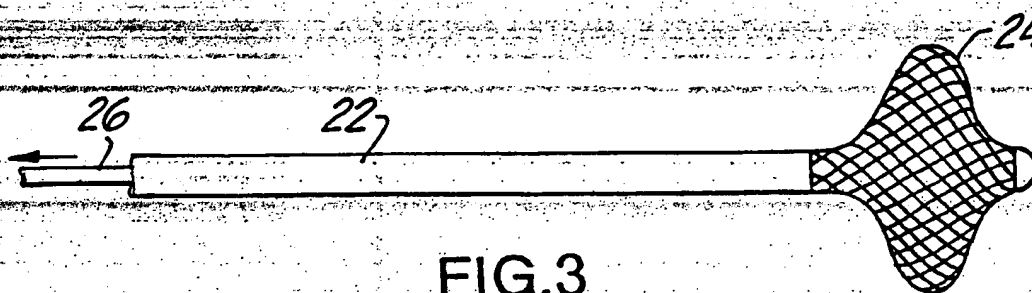


FIG. 3

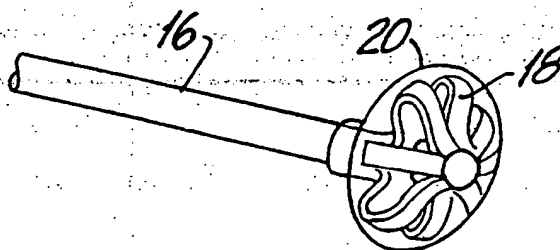


FIG. 4

3/4

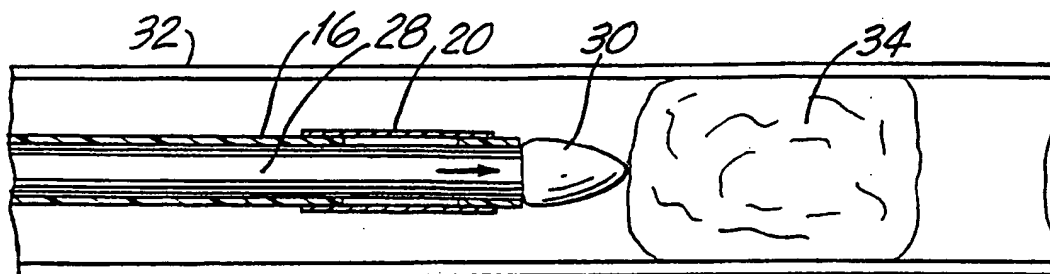


FIG. 5

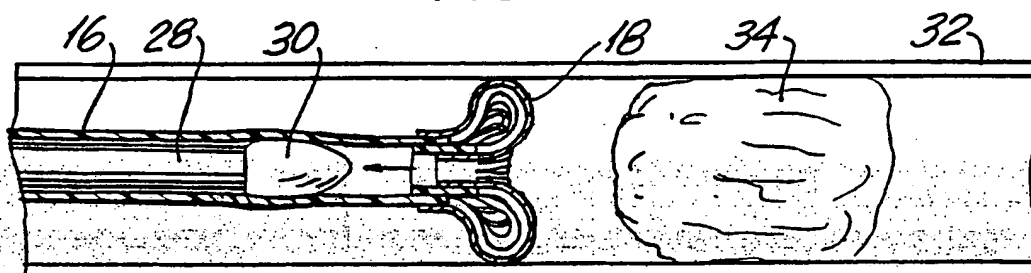


FIG. 6

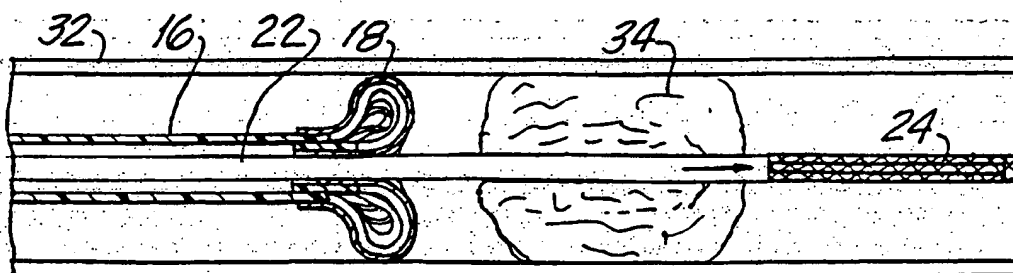


FIG. 7

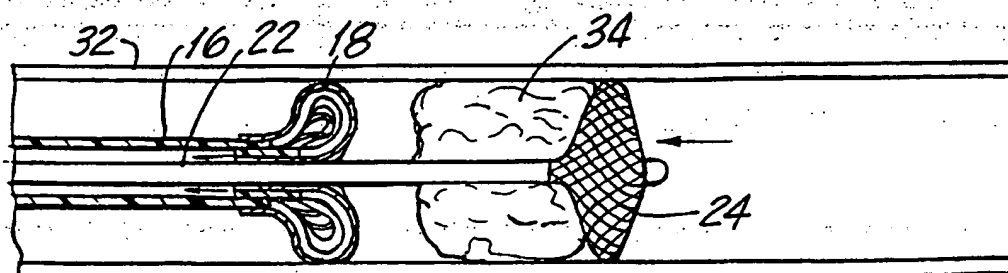


FIG. 8

4/4

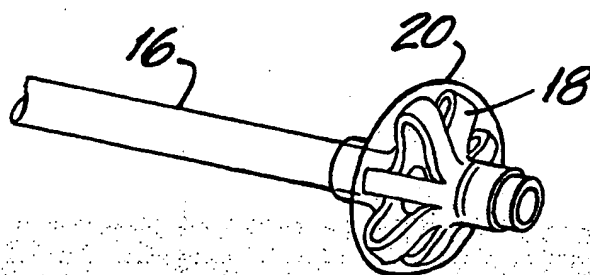


FIG. 9

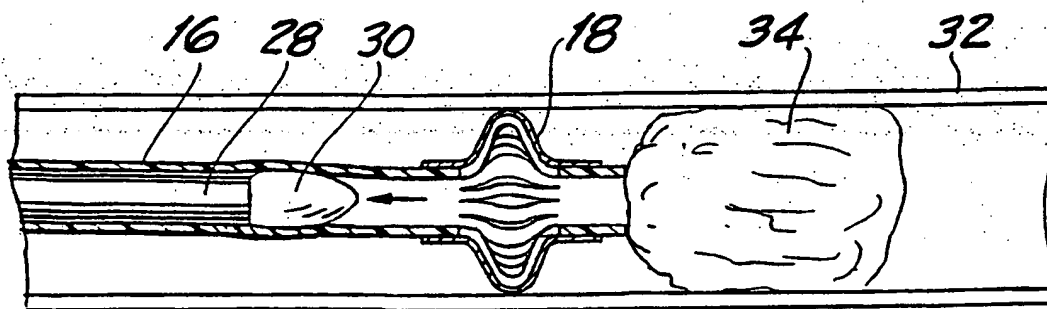


FIG. 10

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US98/23846

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) : A61B 17/00

US CL : 606/108, 194, 200

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 606/108, 194, 200

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 5,329,942 A (GUNTHER et al.) 19 July 1994, entire document.	1-25

☐ Further documents are listed in the continuation of Box C. ☐ See patent family annex.

*A*	document defining the general state of the art which is not considered to be of particular relevance	*T*	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
*E*	earlier document published on or after the international filing date	*X*	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
*L*	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*Y*	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
*O*	document referring to an oral disclosure, use, exhibition or other means	*Z*	document member of the same patent family
*P*	document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search

16 JANUARY 1999

Date of mailing of the international search report

29 JAN 1999

Name and mailing address of the ISA/US  
Commissioner of Patents and Trademarks  
Box PCT  
Washington, D.C. 20231

Facsimile No. (703) 308-2708

Authorized officer

VIKKI TRINH

Telephone No. (703) 308-8238

Form PCT/ISA/210 (second sheet)(July 1992) \*

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☒ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☒ OTHER: DIRTY BACKGROUND

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**